

Fig. 1

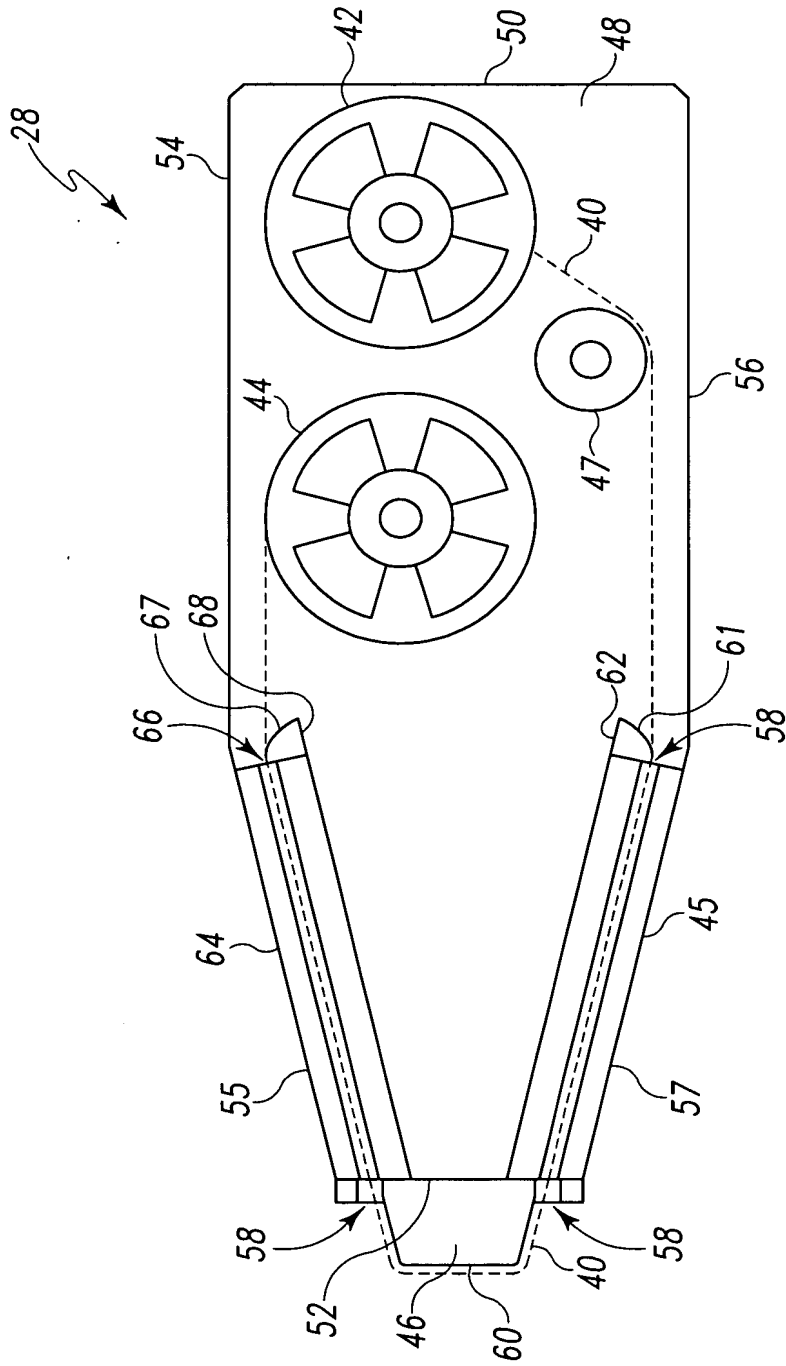
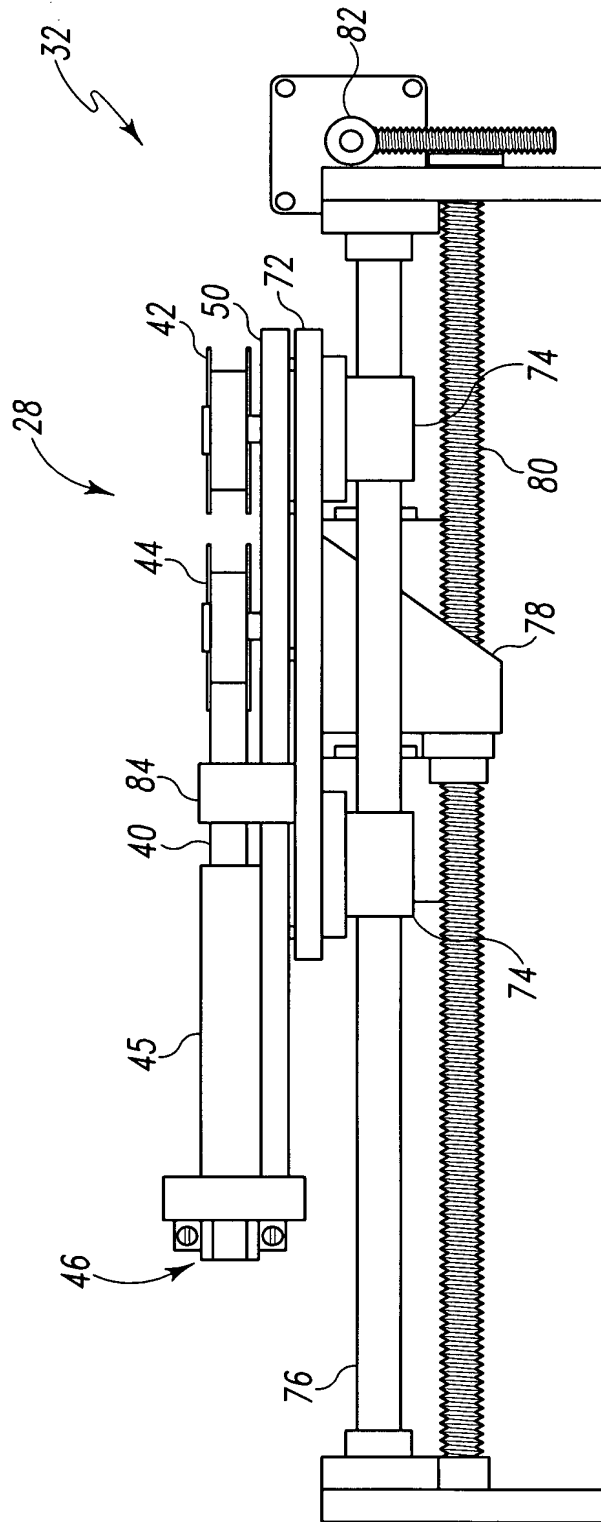


Fig. 2



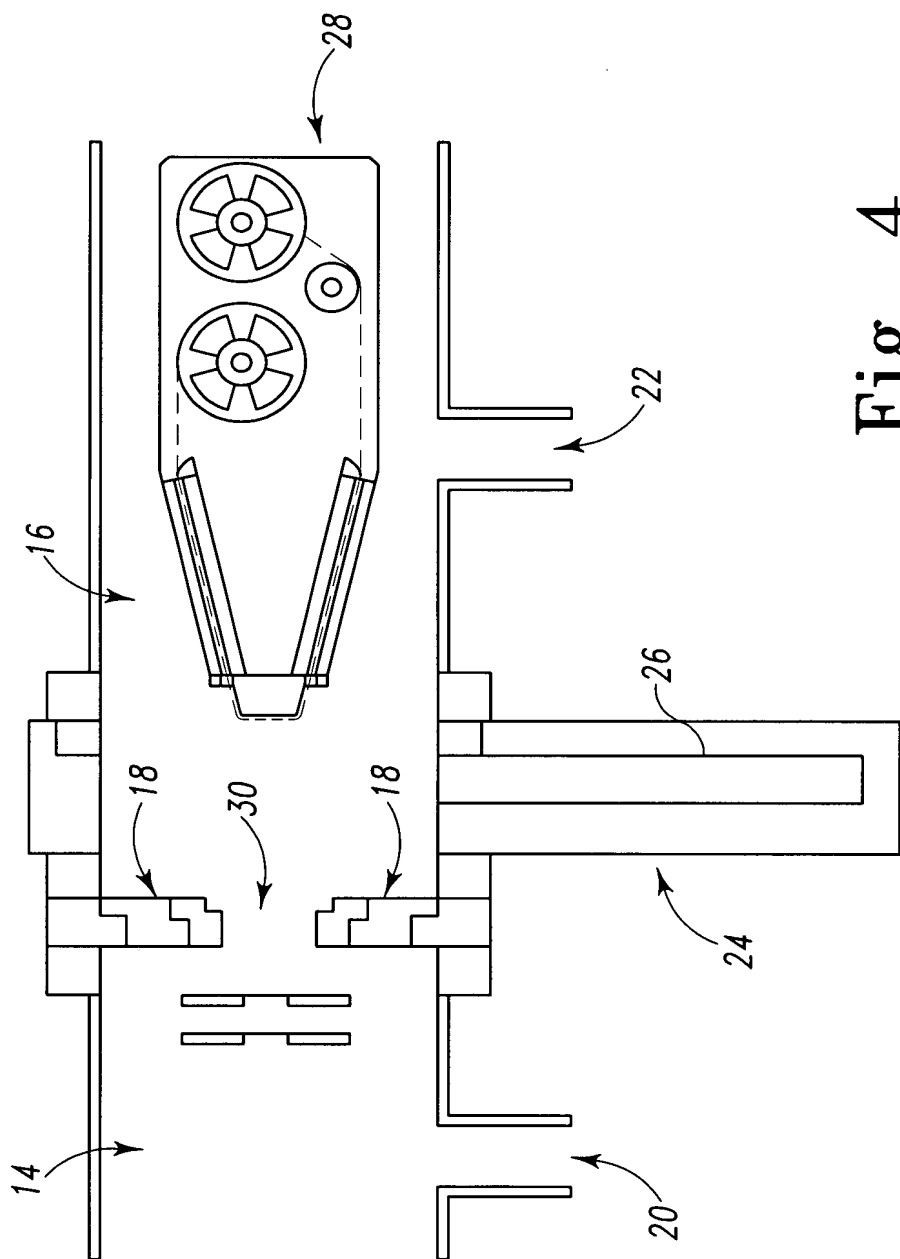


Fig. 4

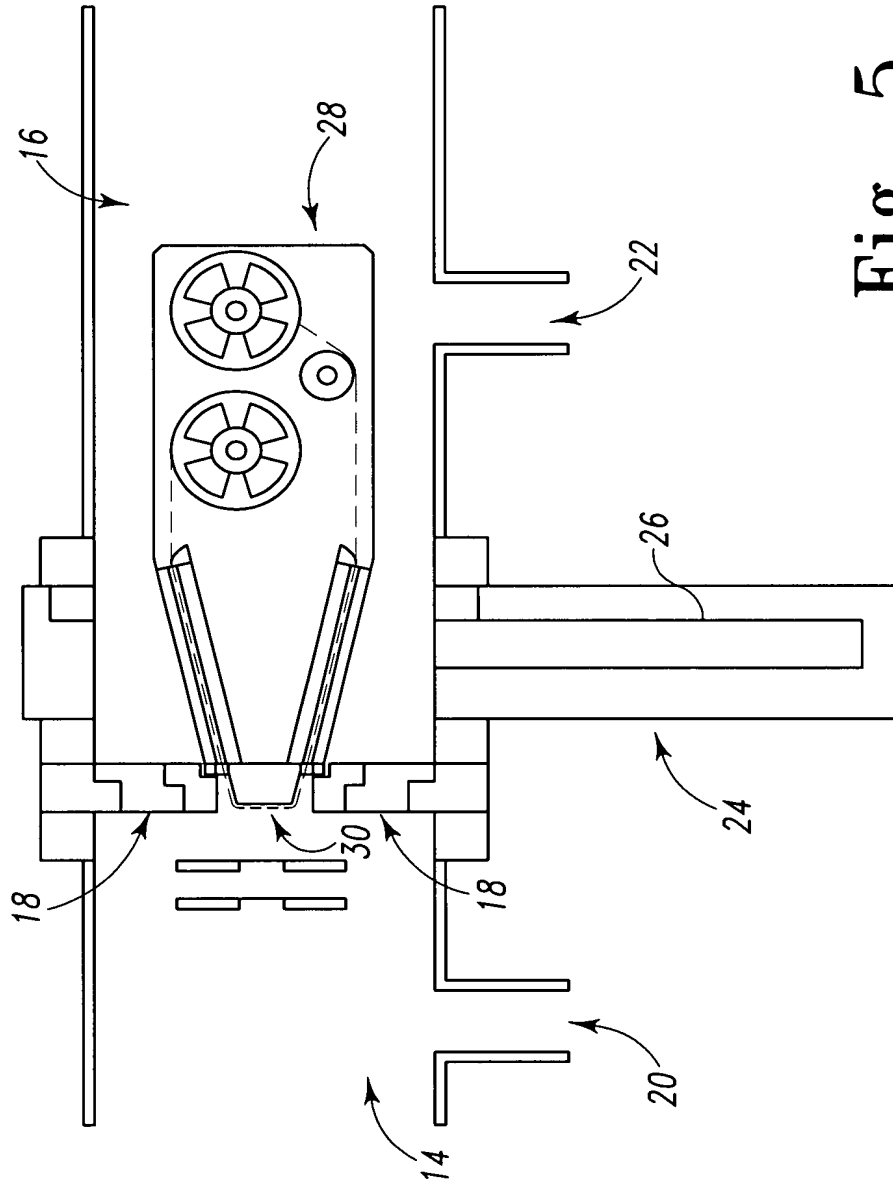


Fig. 5

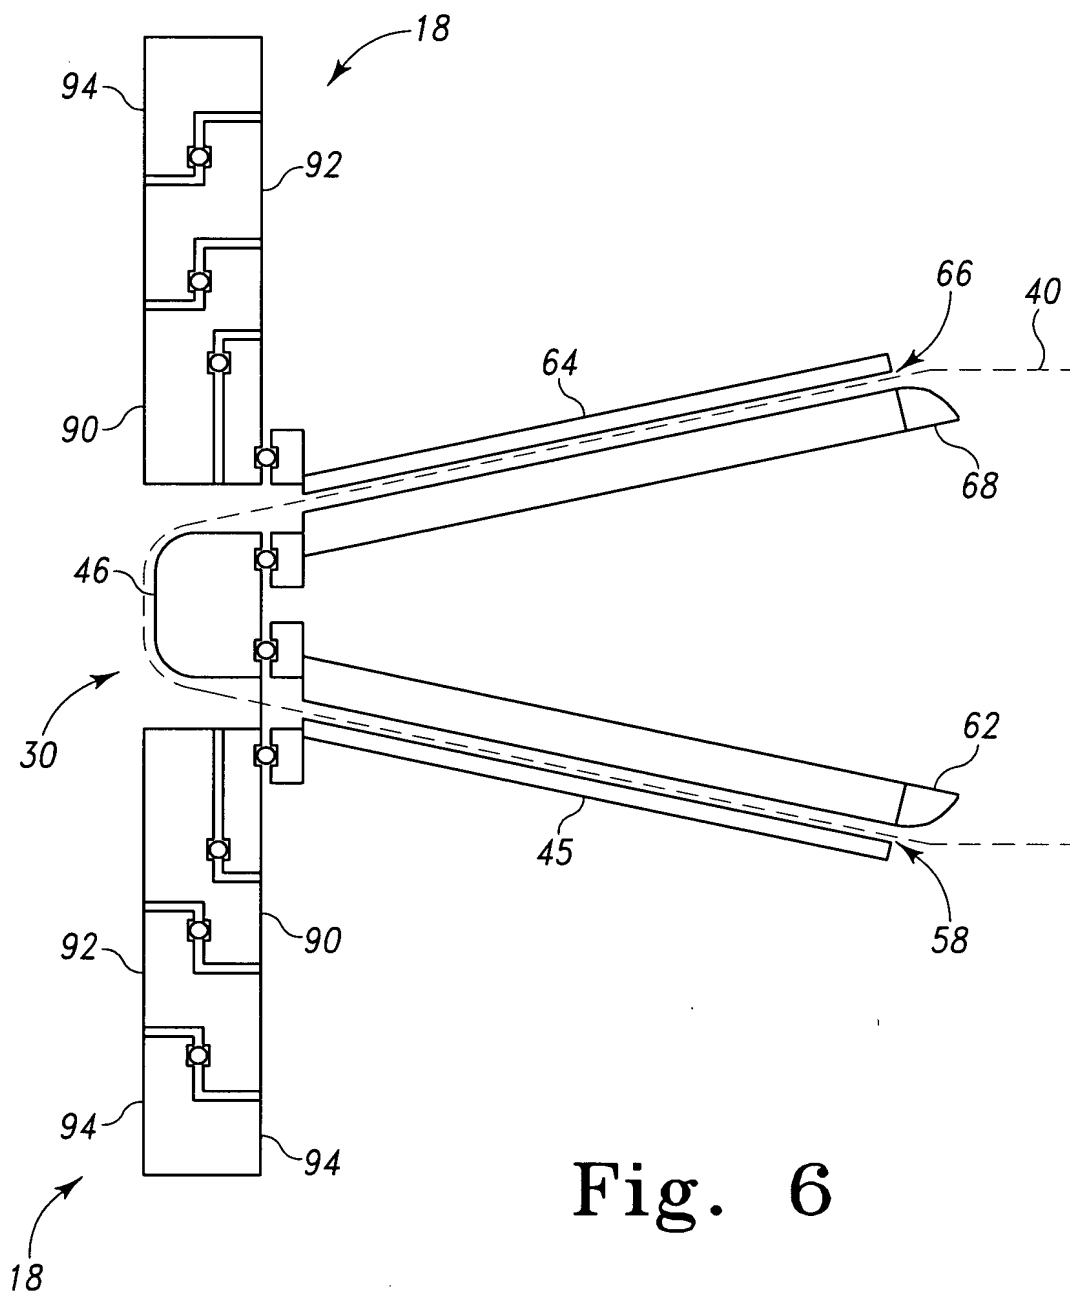


Fig. 6

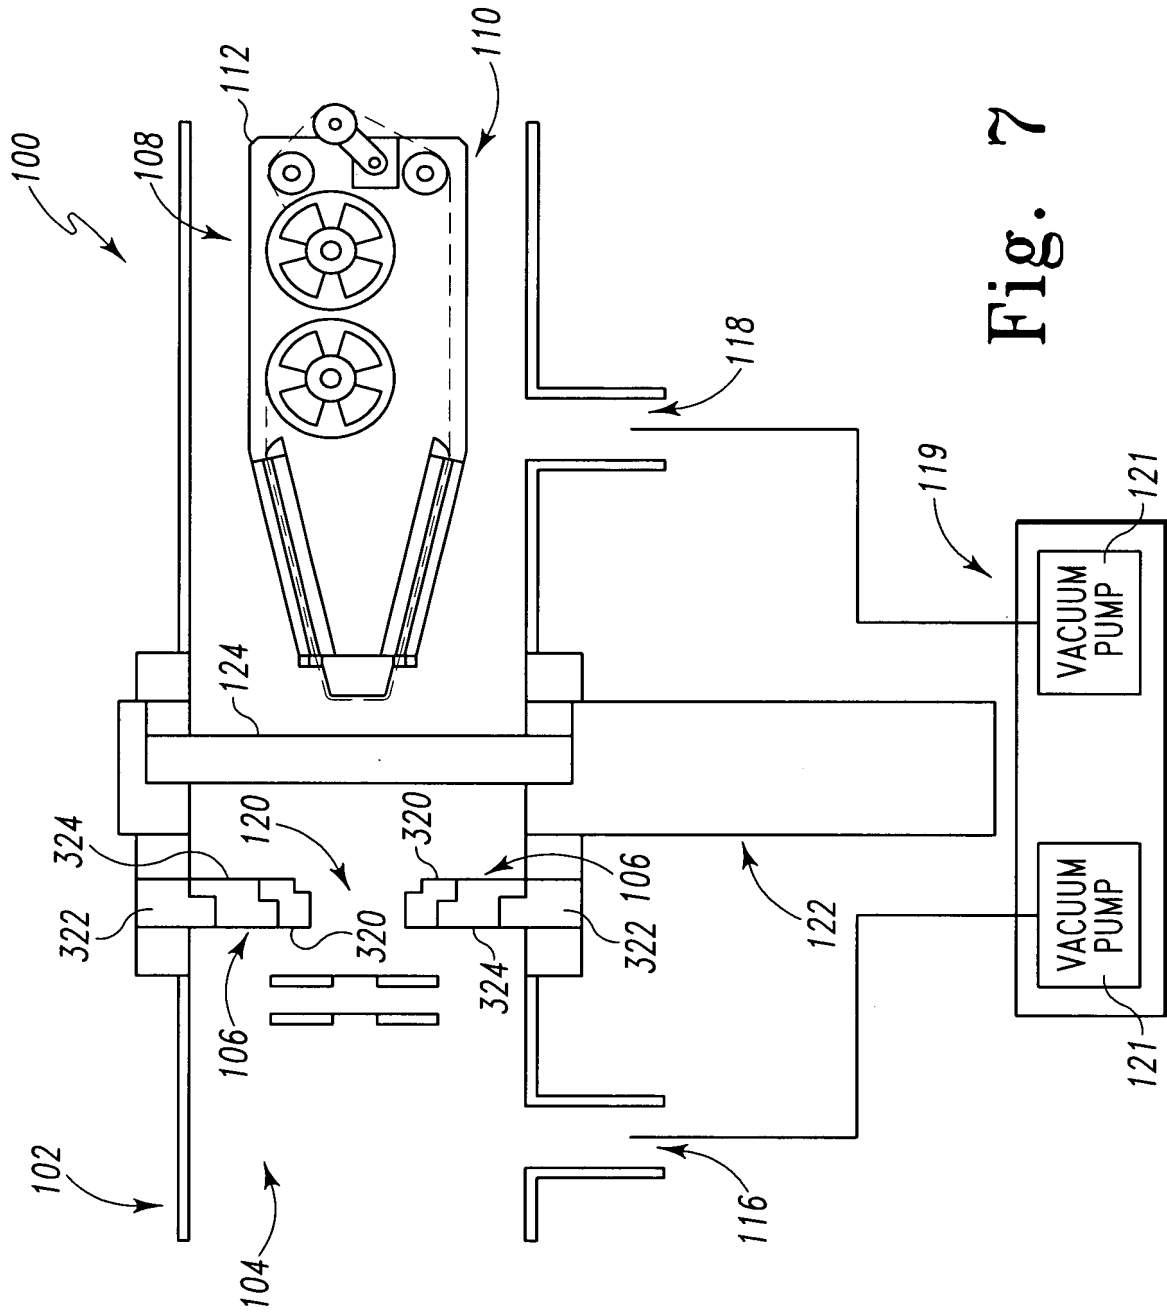


Fig. 7

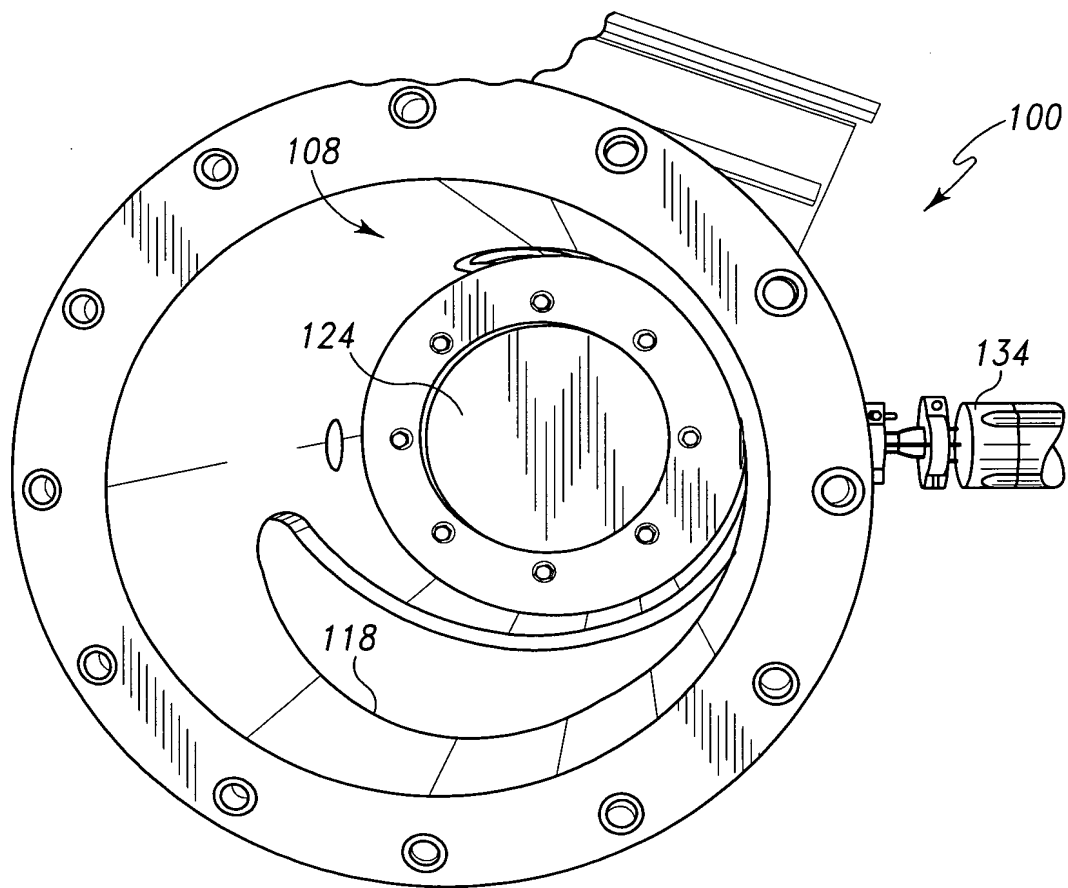


Fig. 8

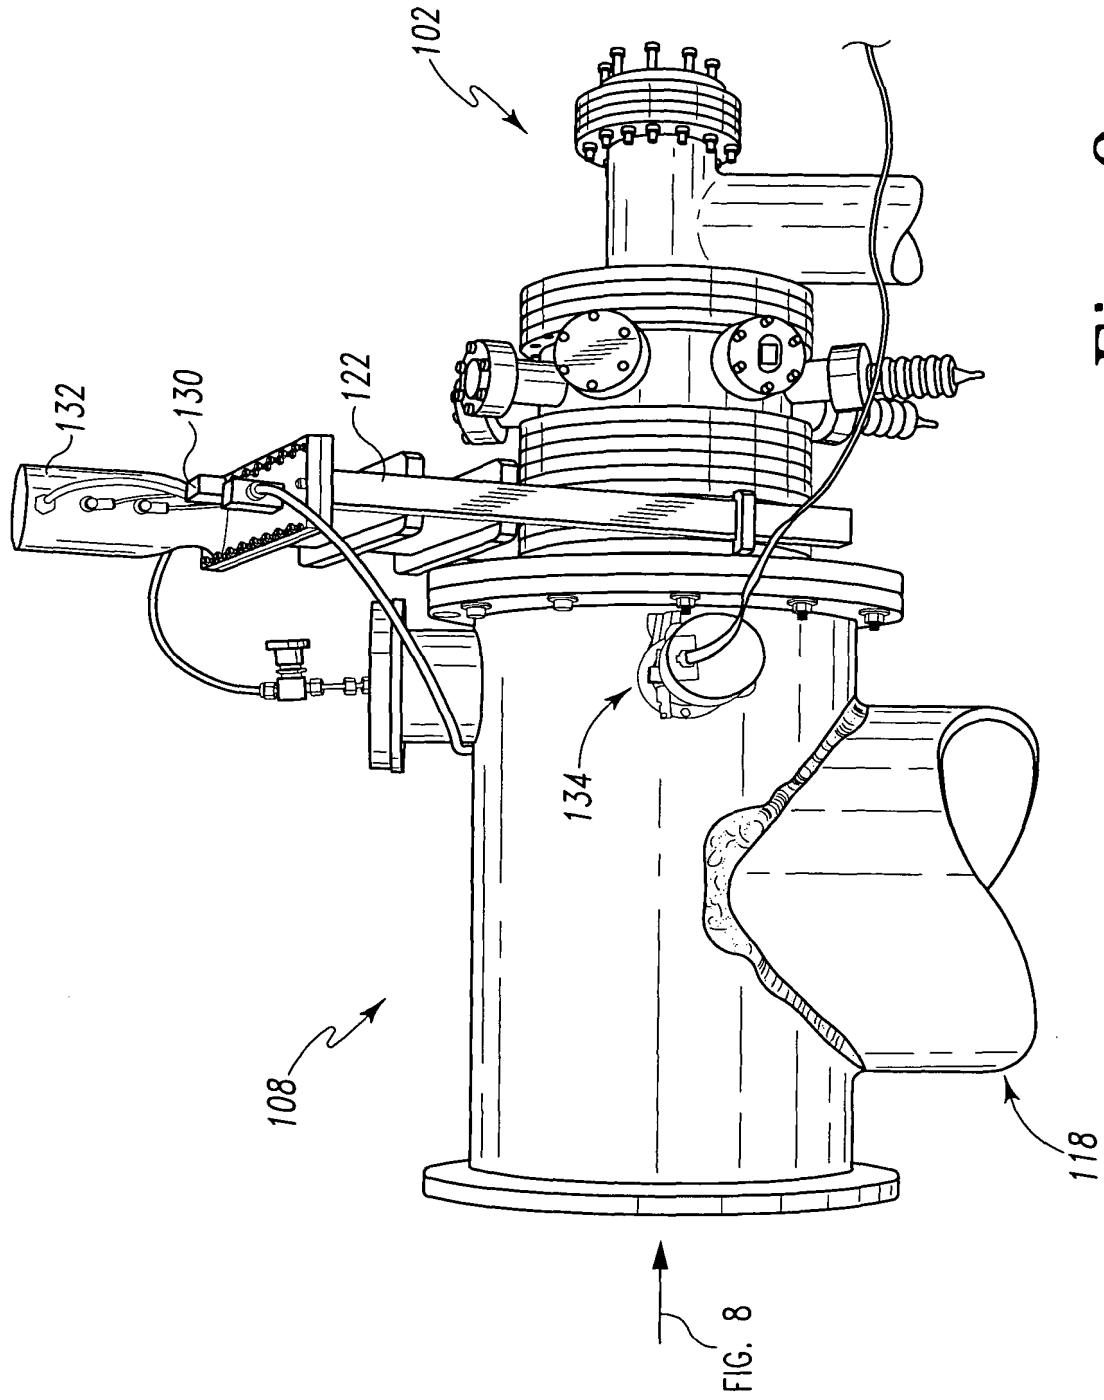


Fig. 9

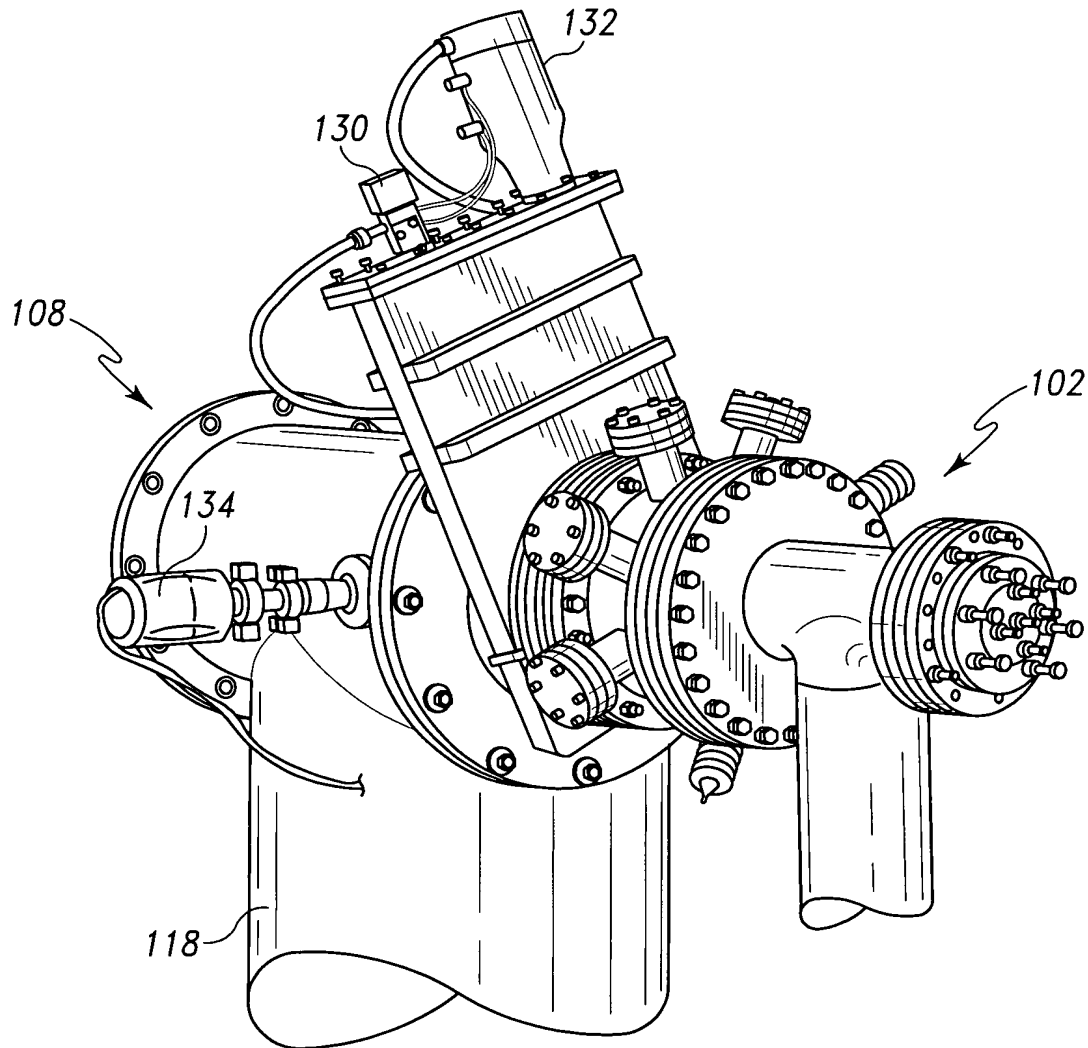


Fig. 10

METHOD AND APPARATUS FOR MASS
SPECTROMETRIC ANALYSIS OF SAMPLES

James P. Reilly et al.
29920-72731/ARTI-0311

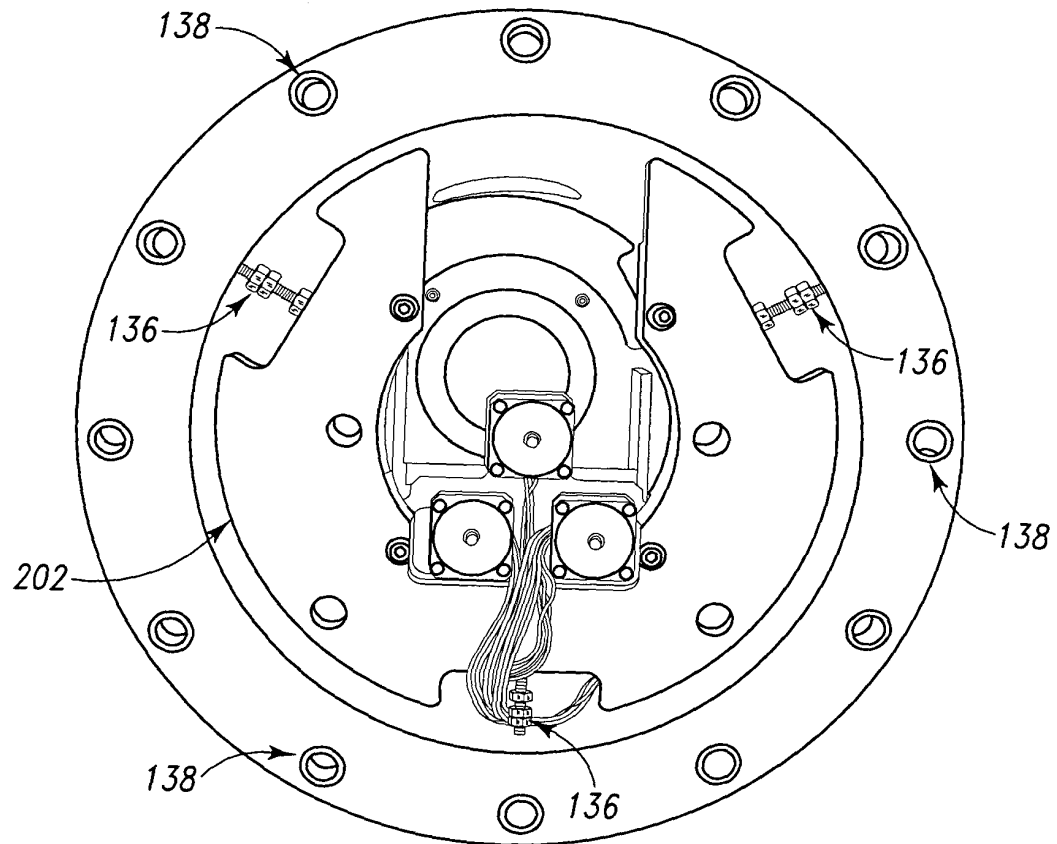


Fig. 11

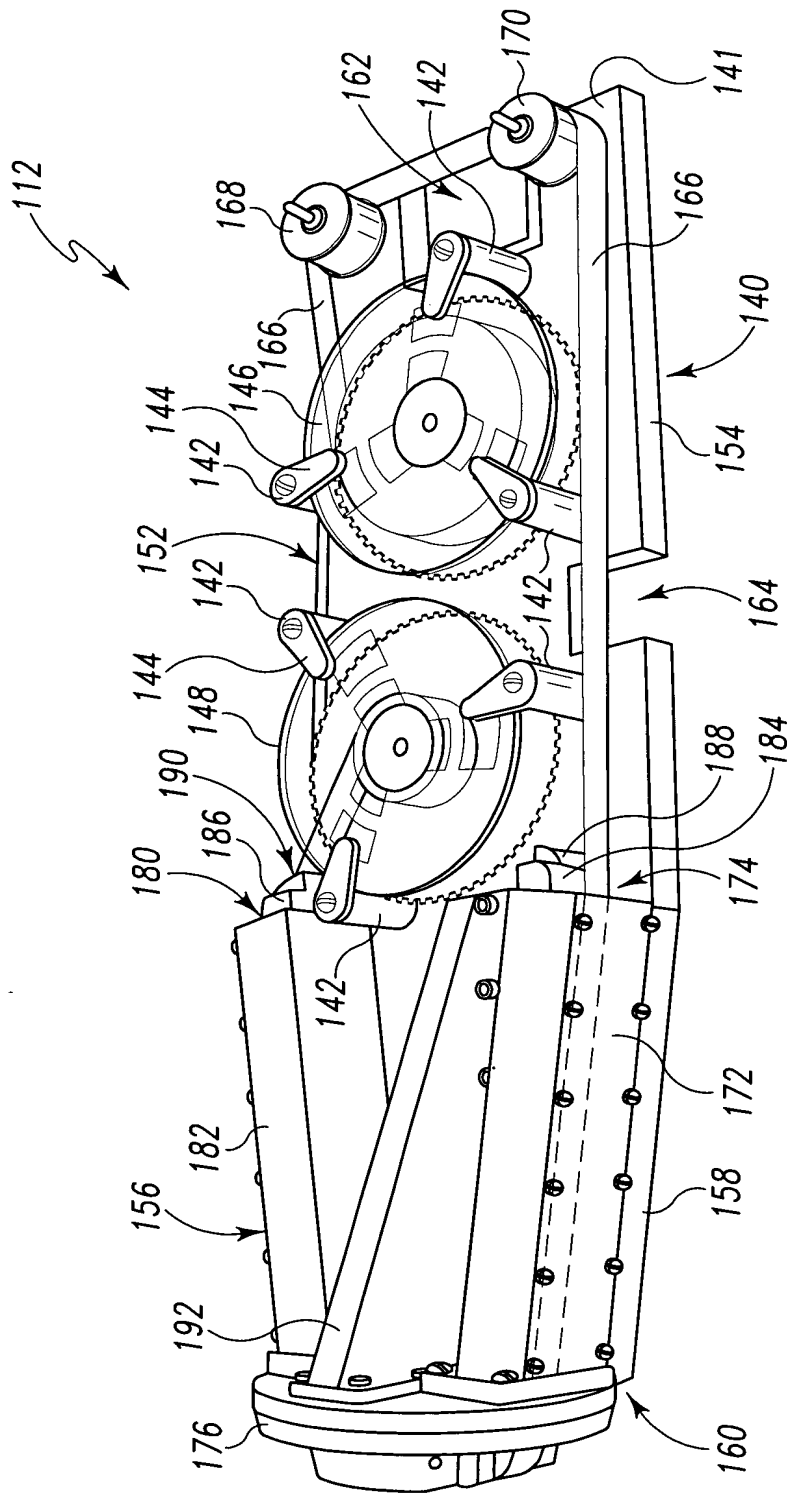


Fig. 12

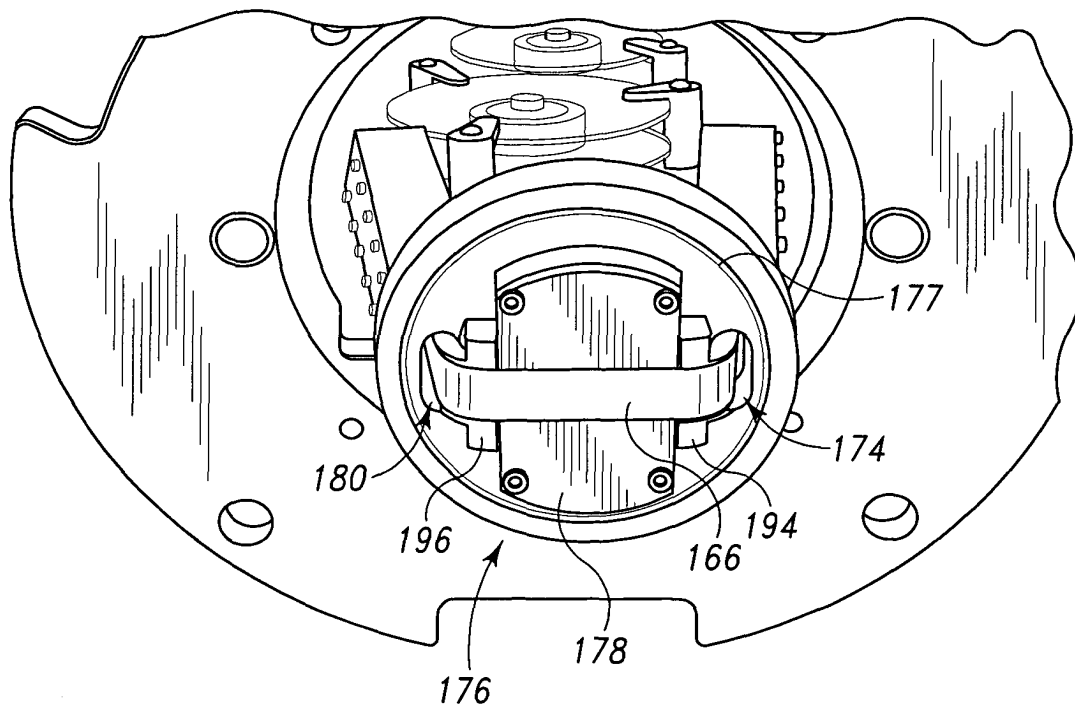
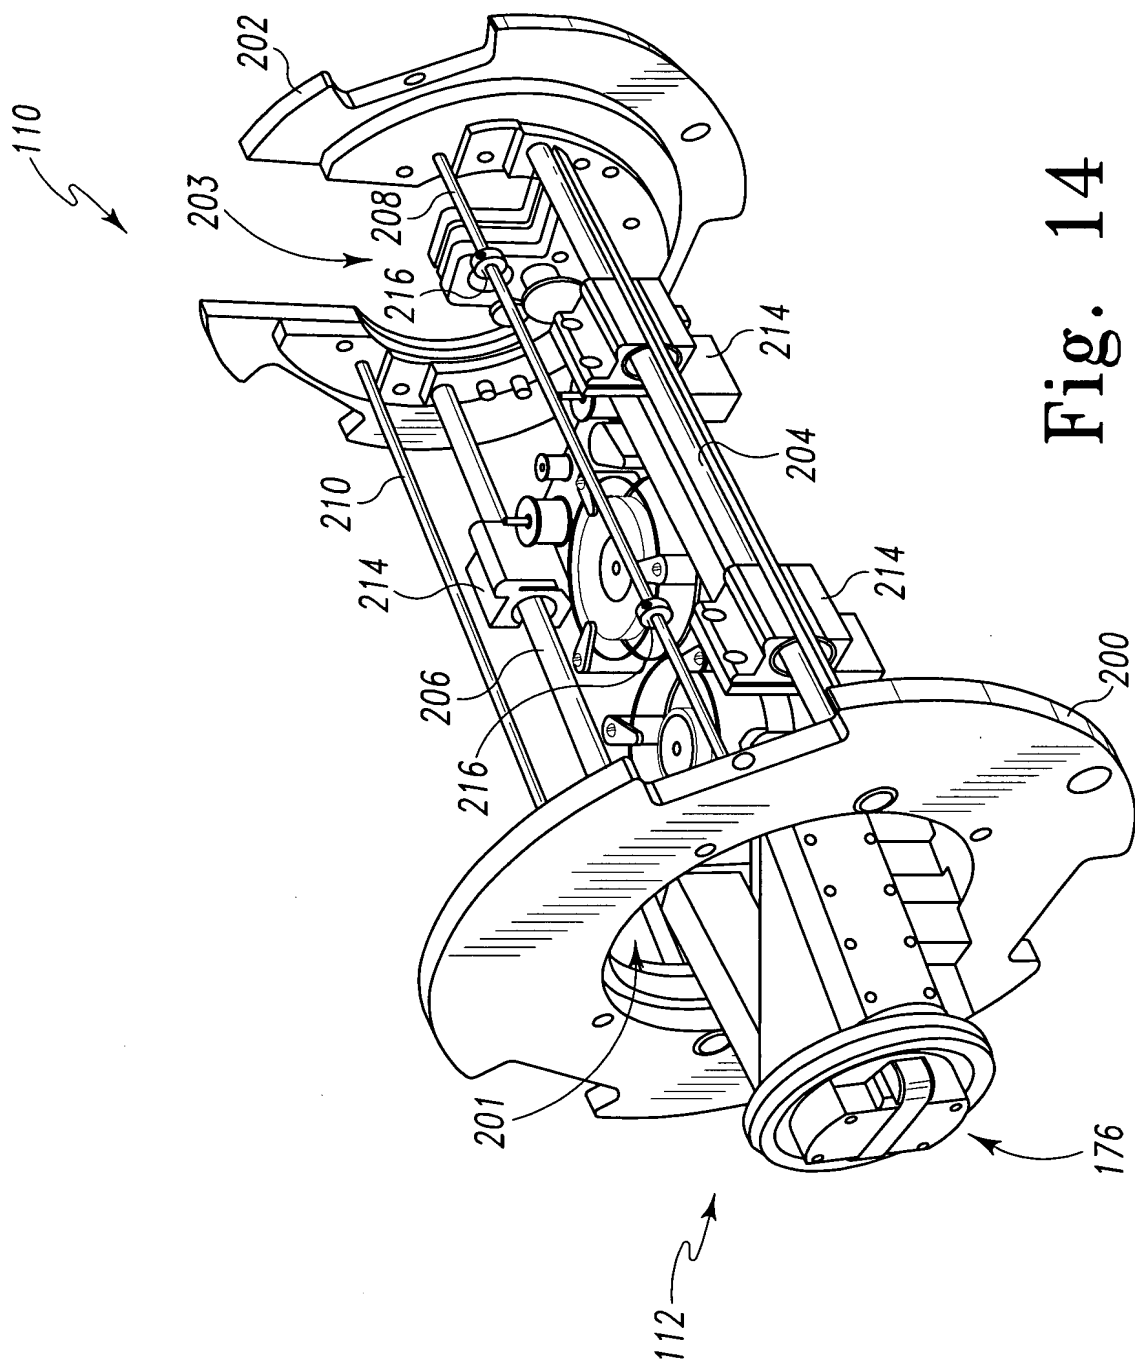


Fig. 13



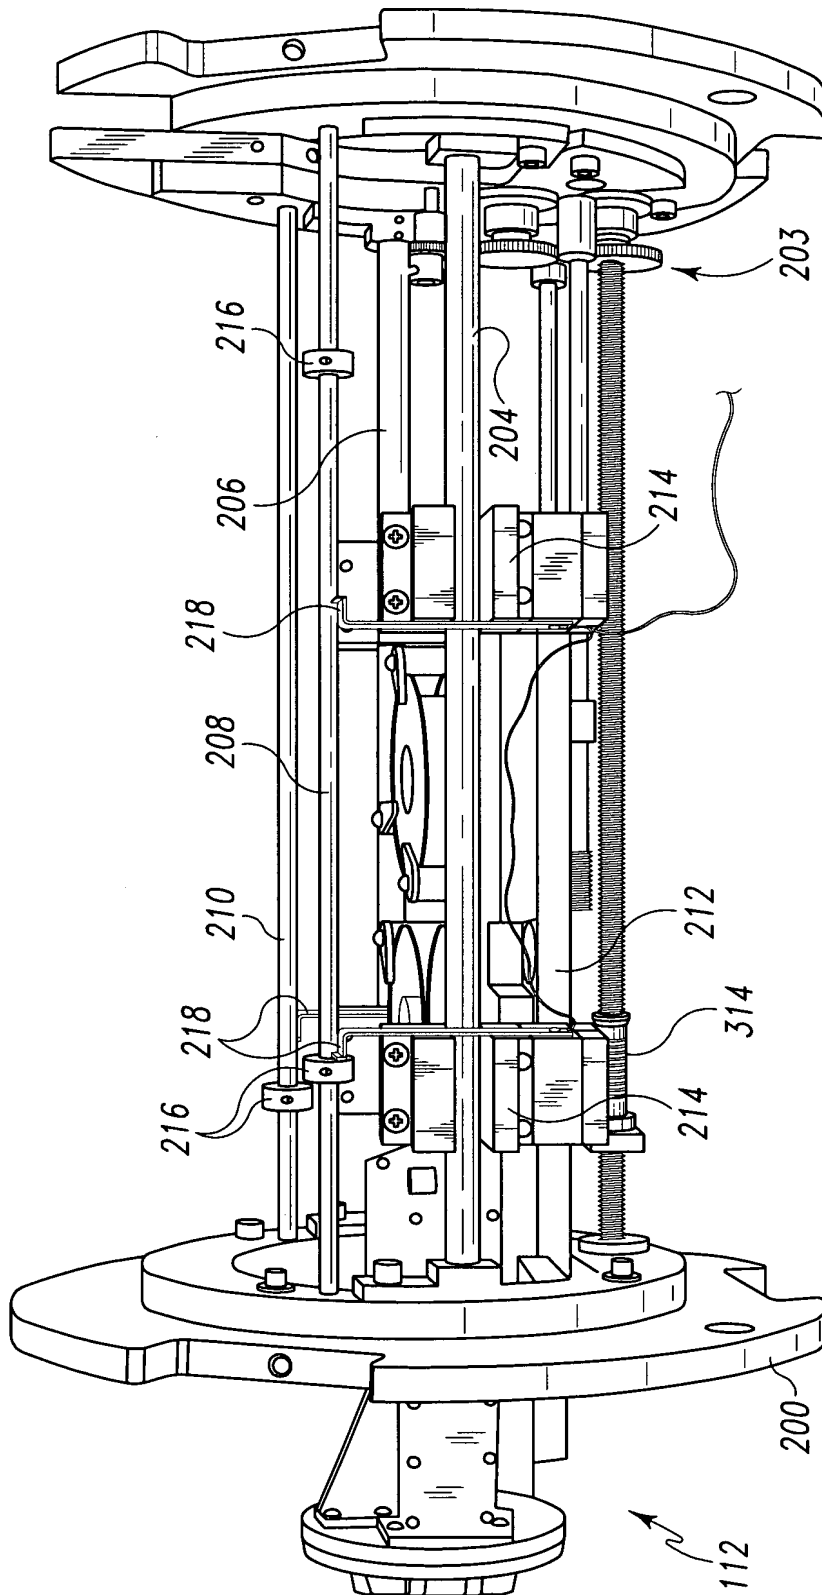


Fig. 15

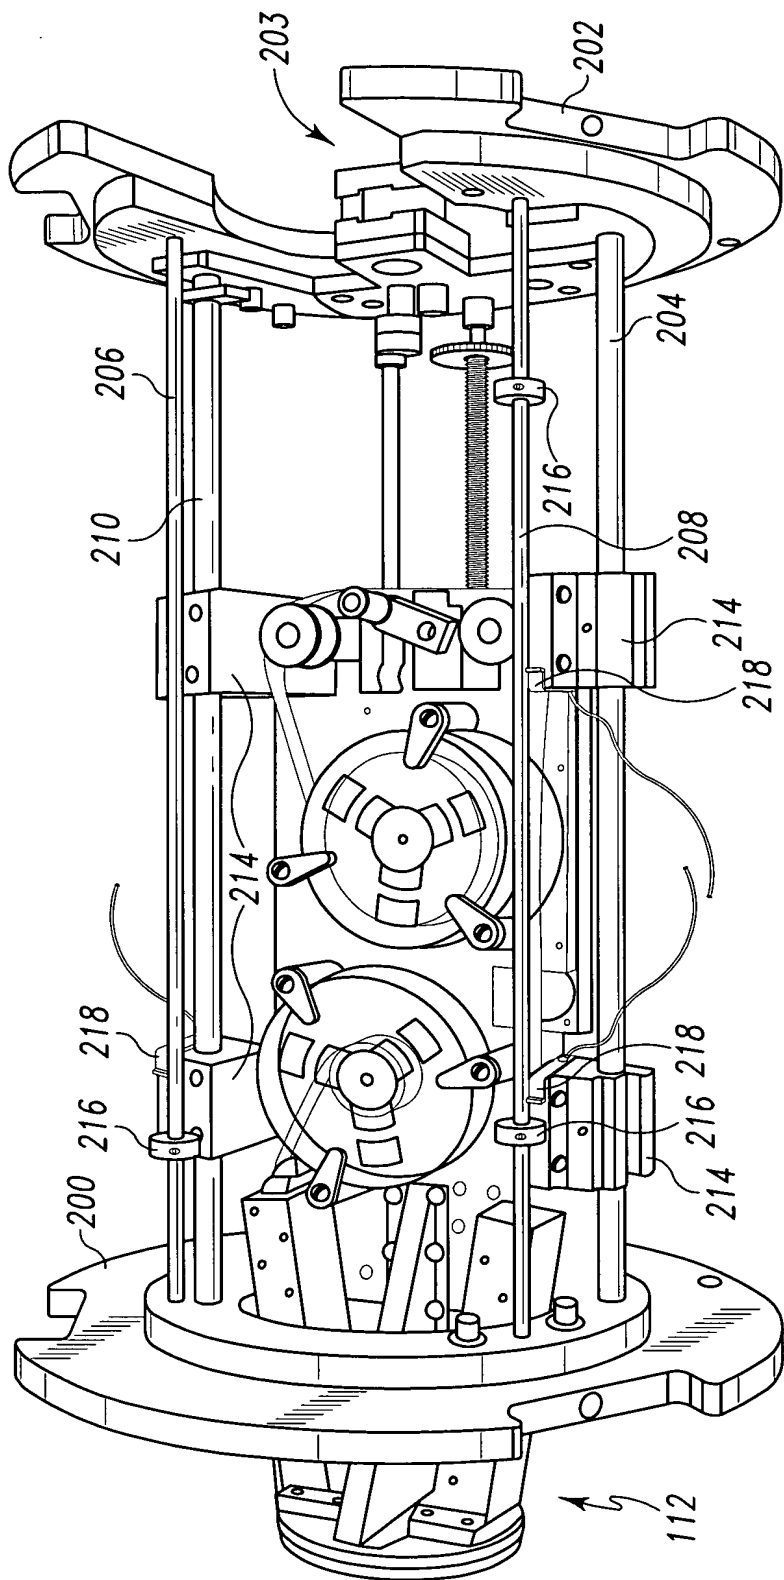


Fig. 16

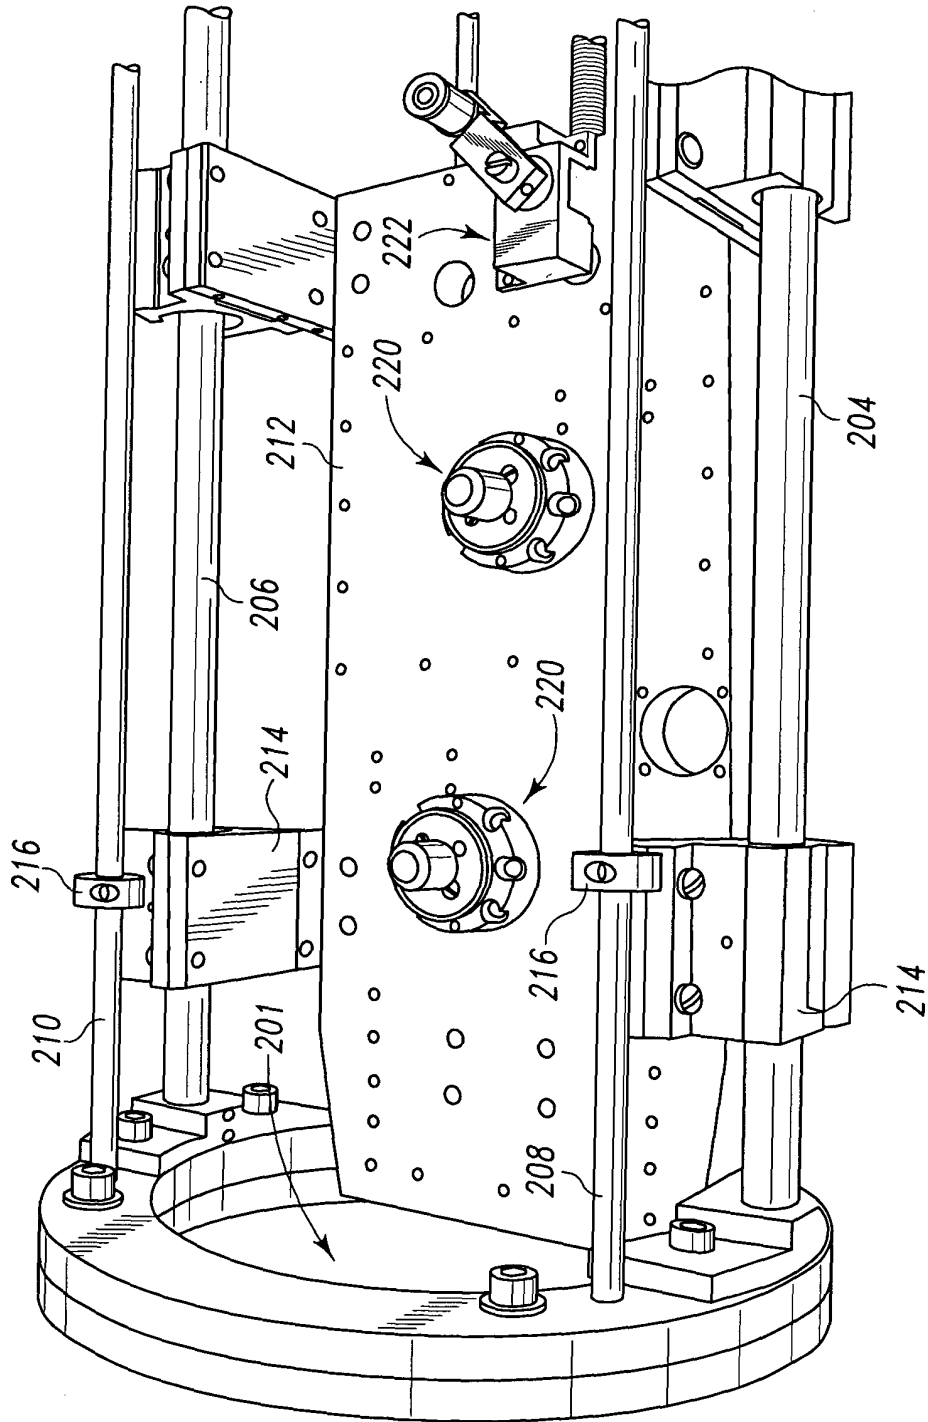


Fig. 17

Fig. 18

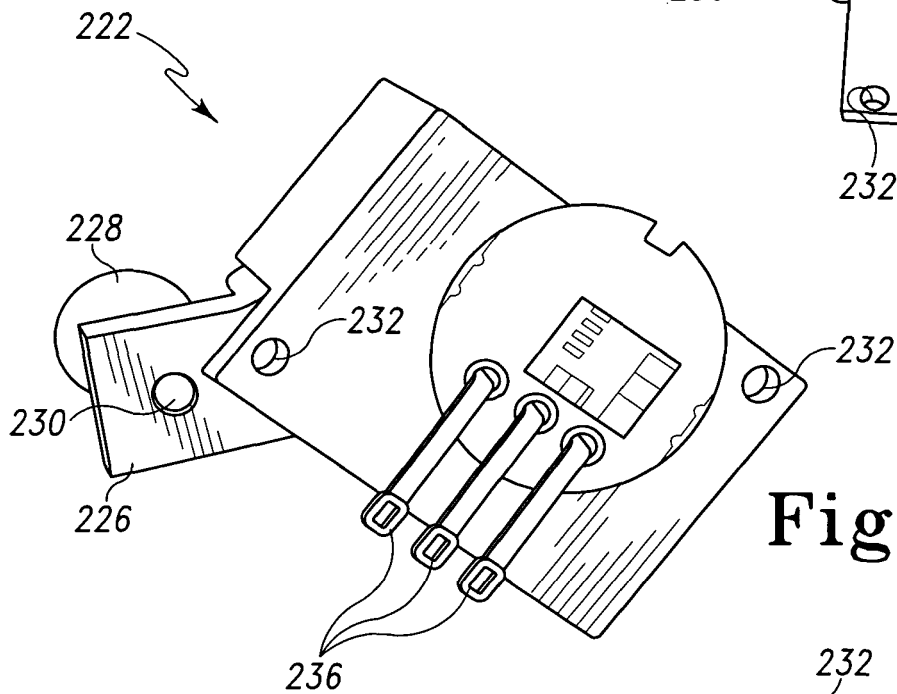
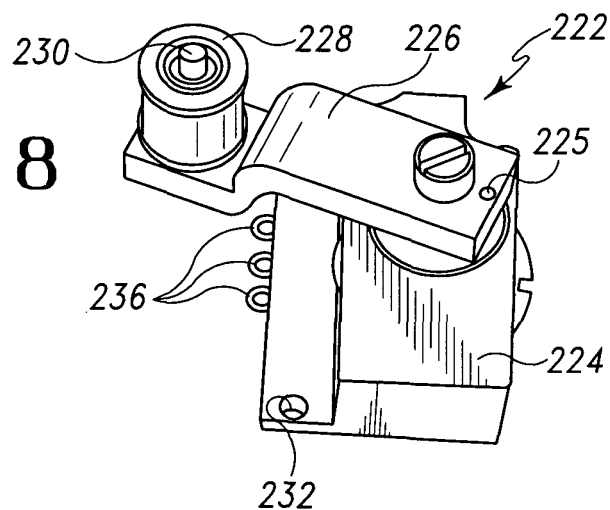


Fig. 19

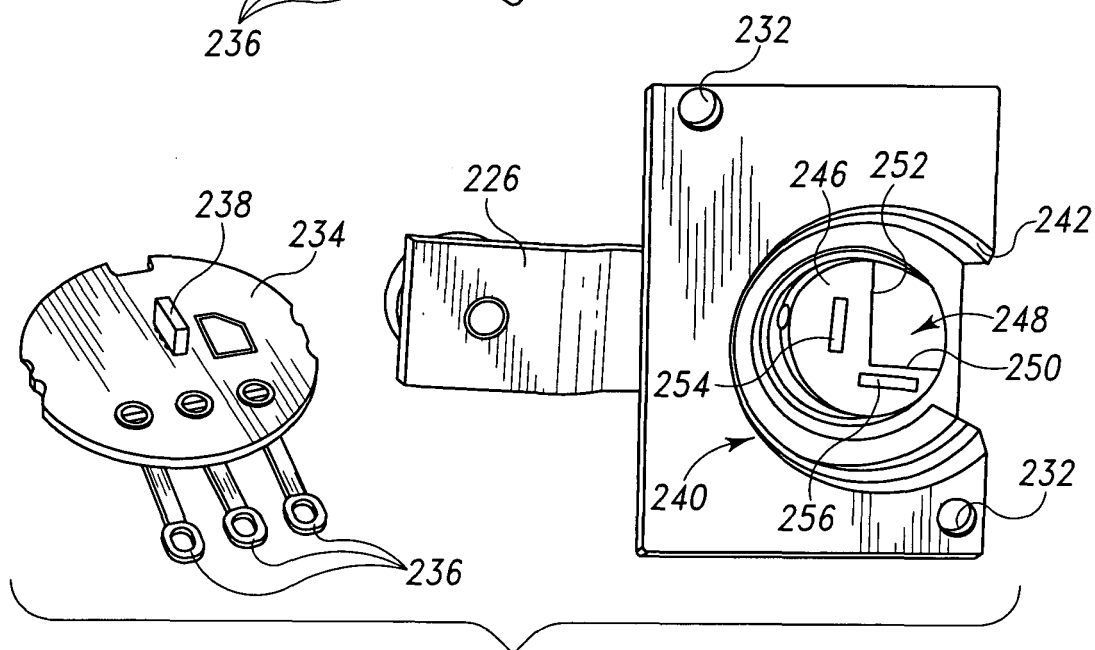


Fig. 20

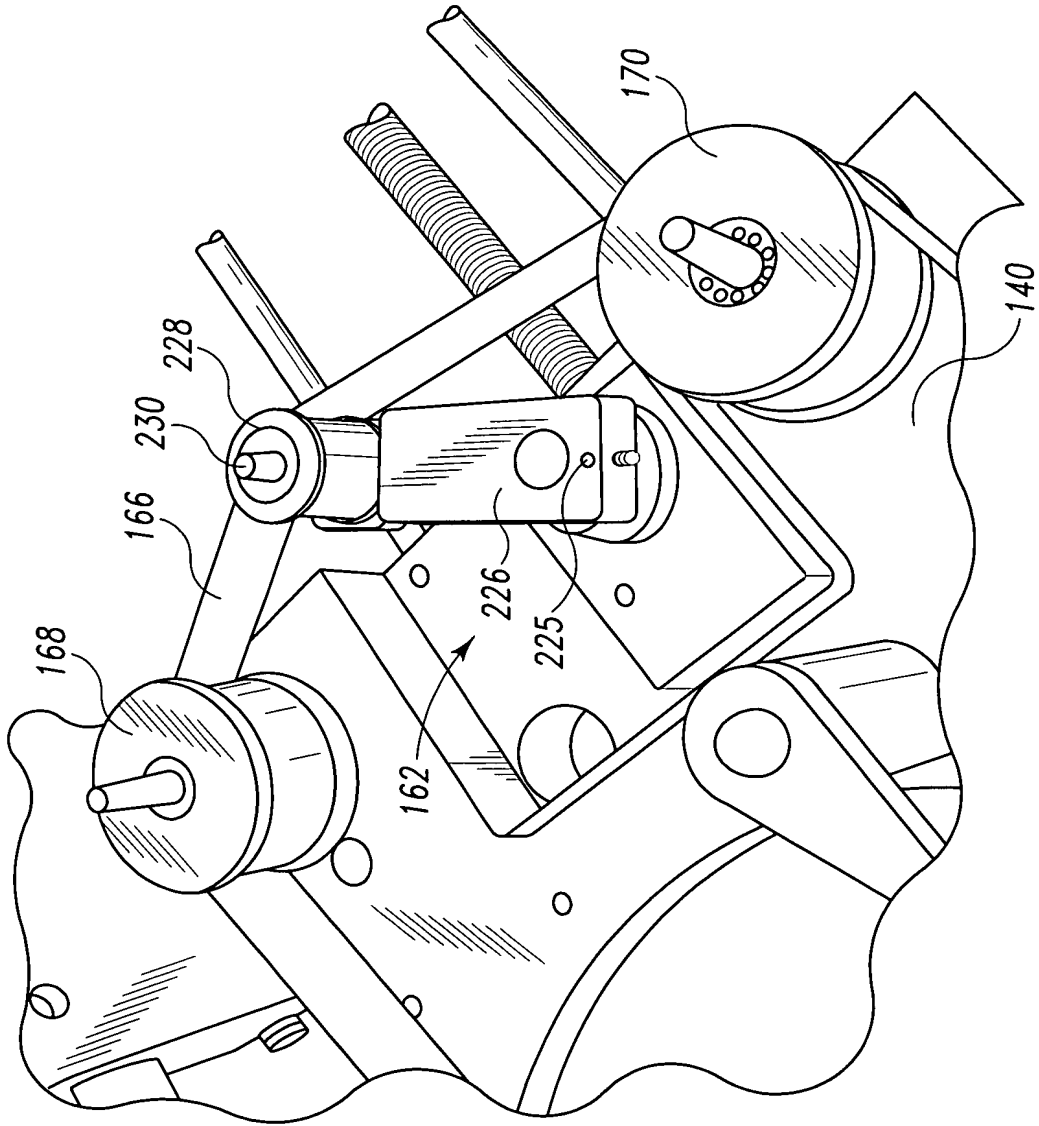


Fig. 21

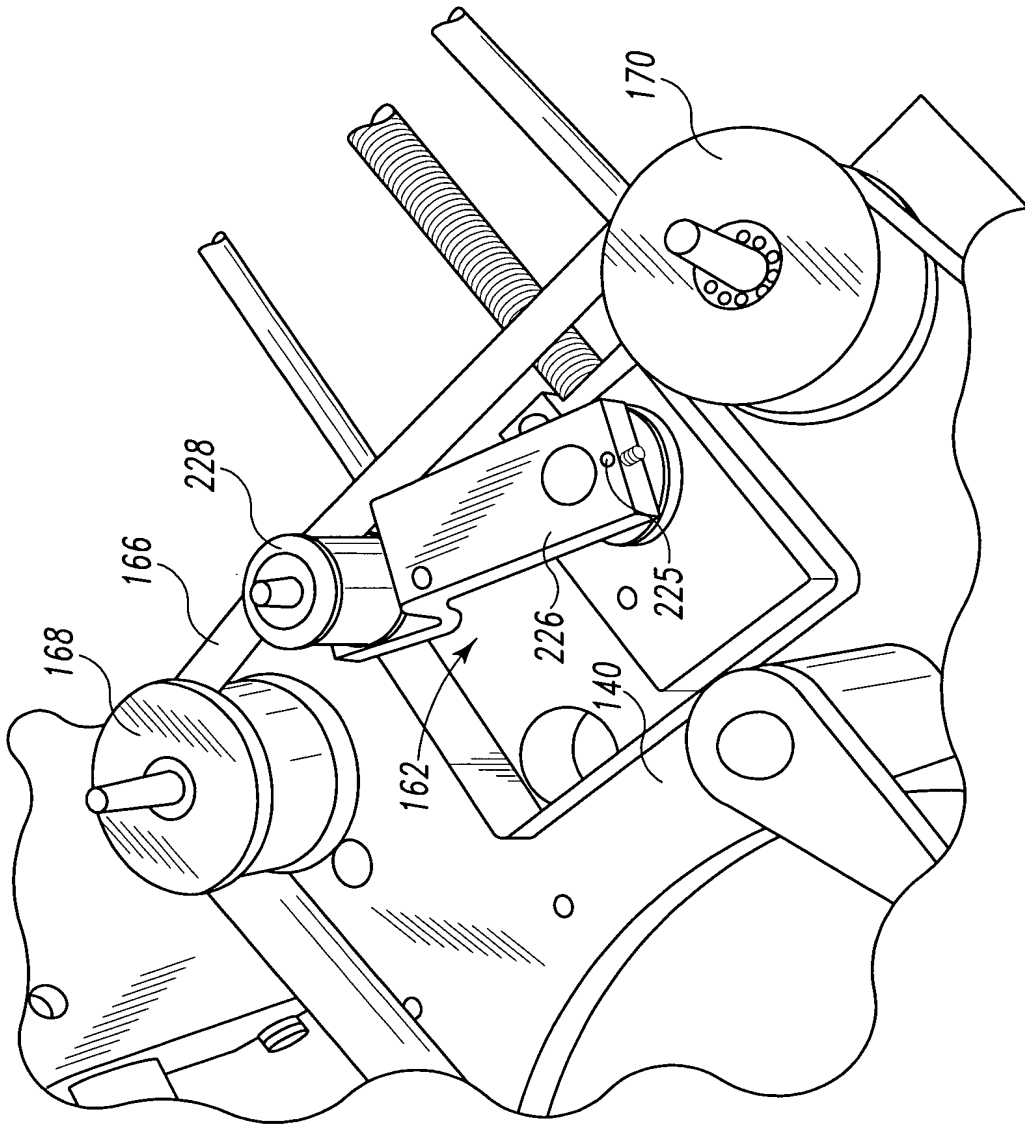


Fig. 22

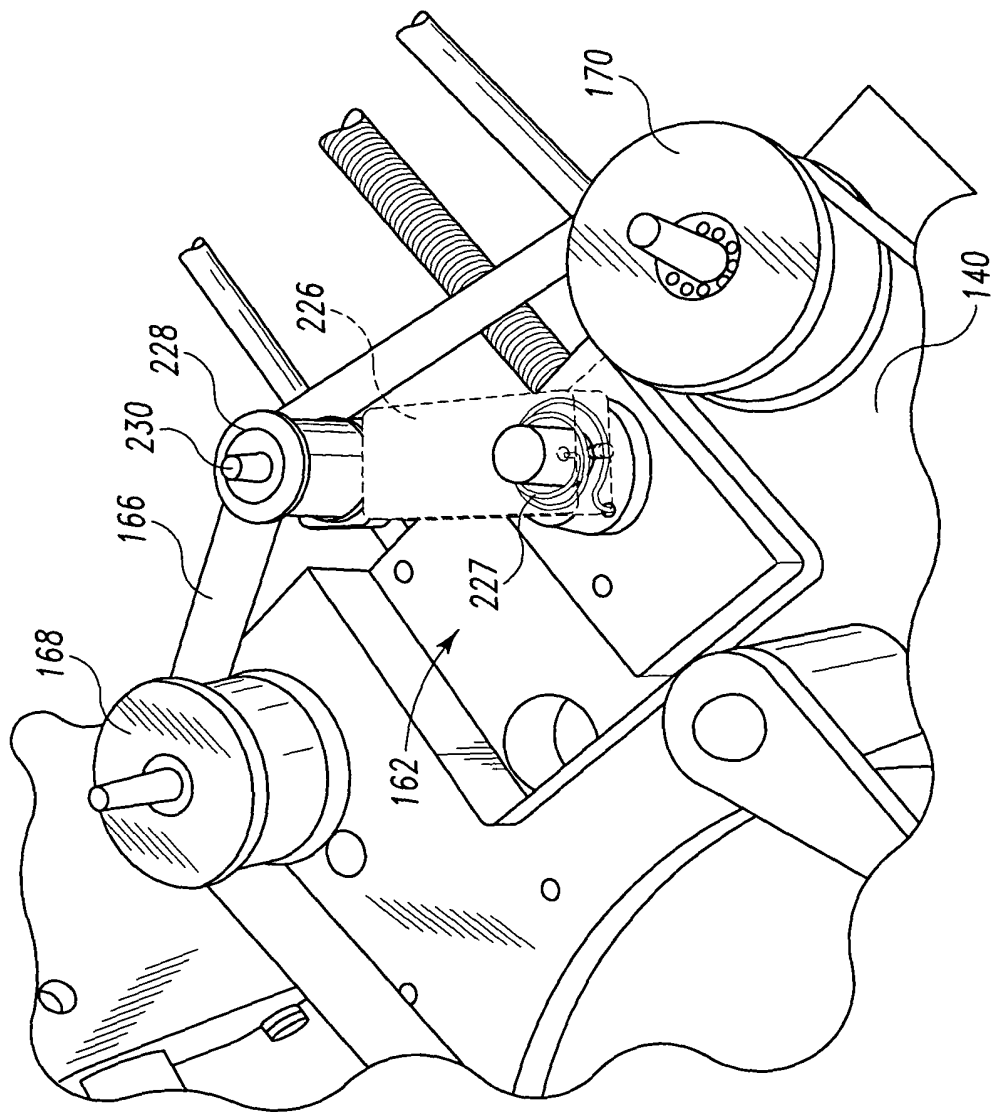


Fig. 23

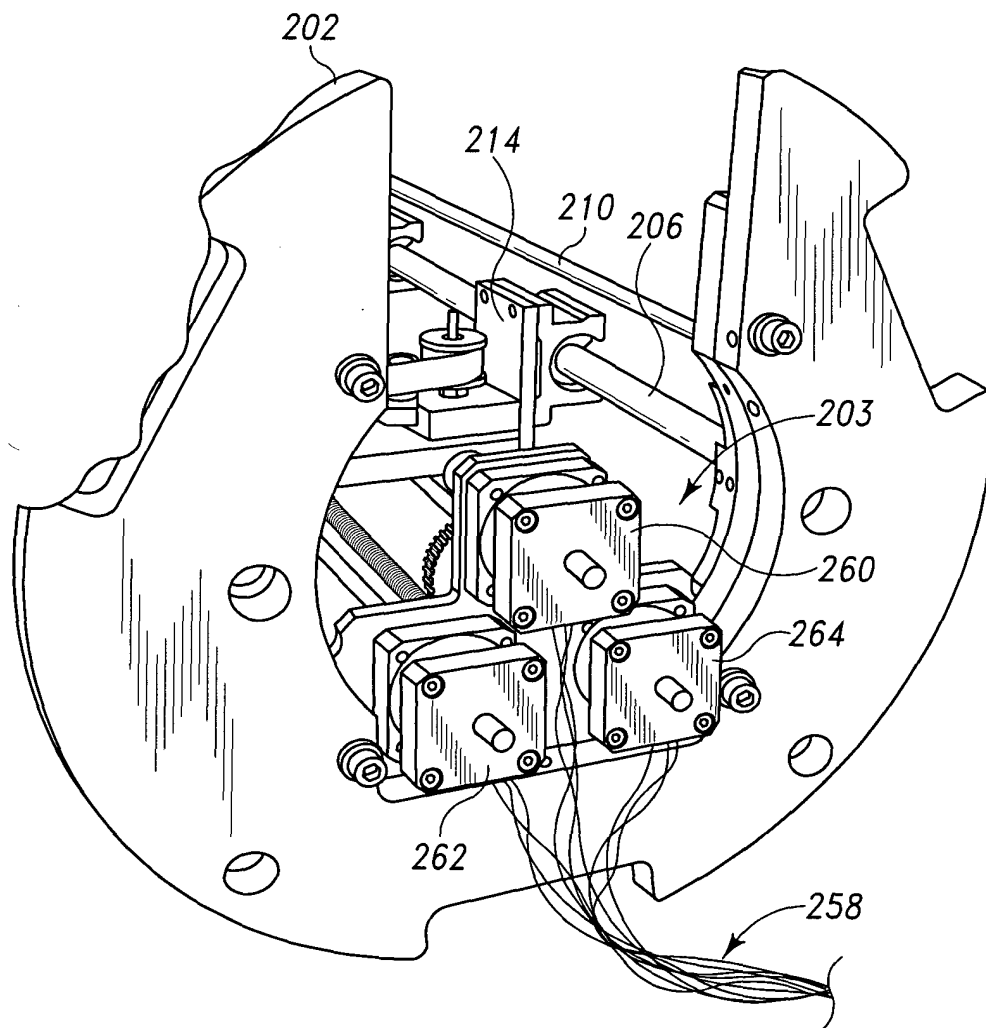


Fig. 24

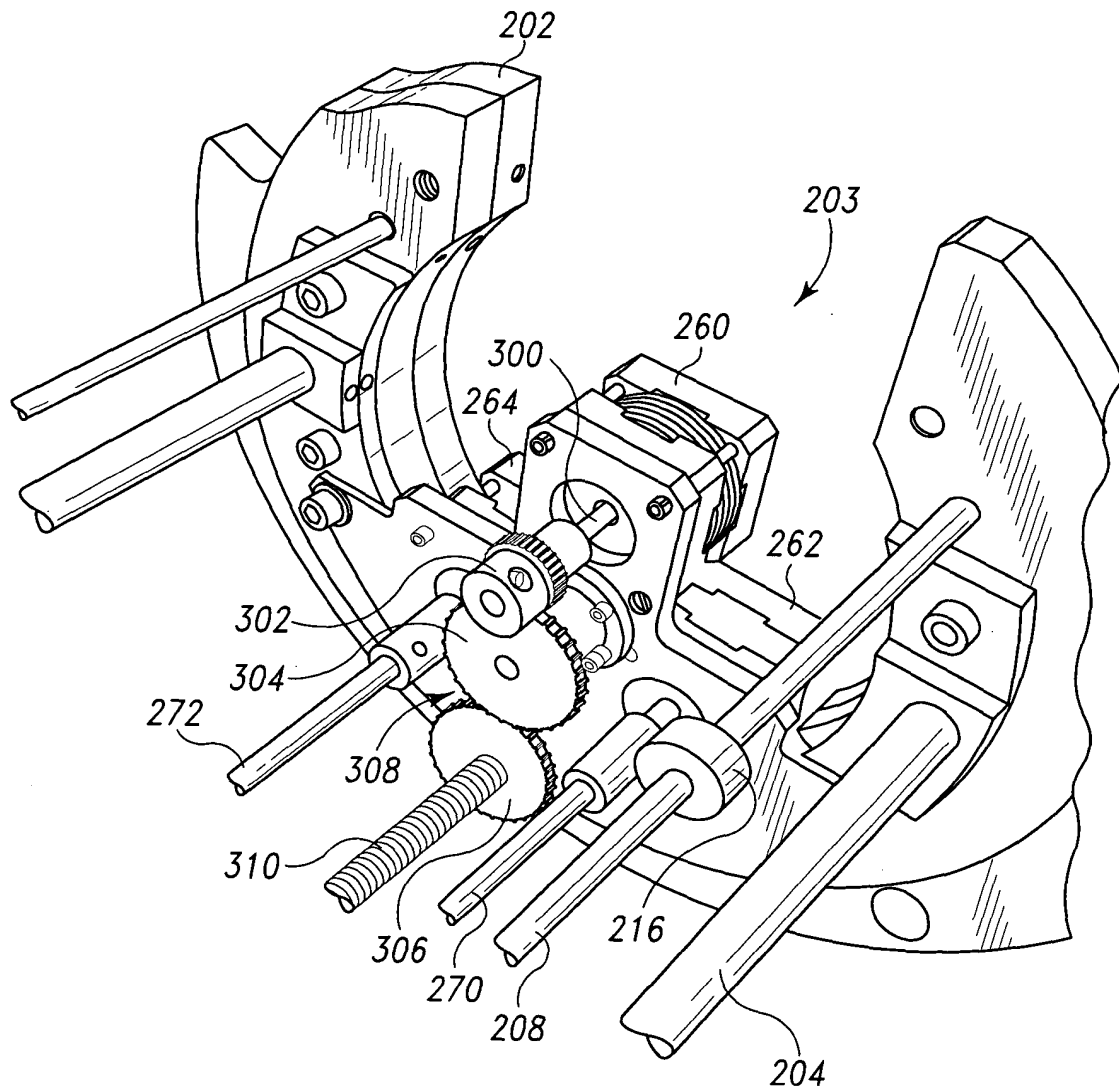


Fig. 25

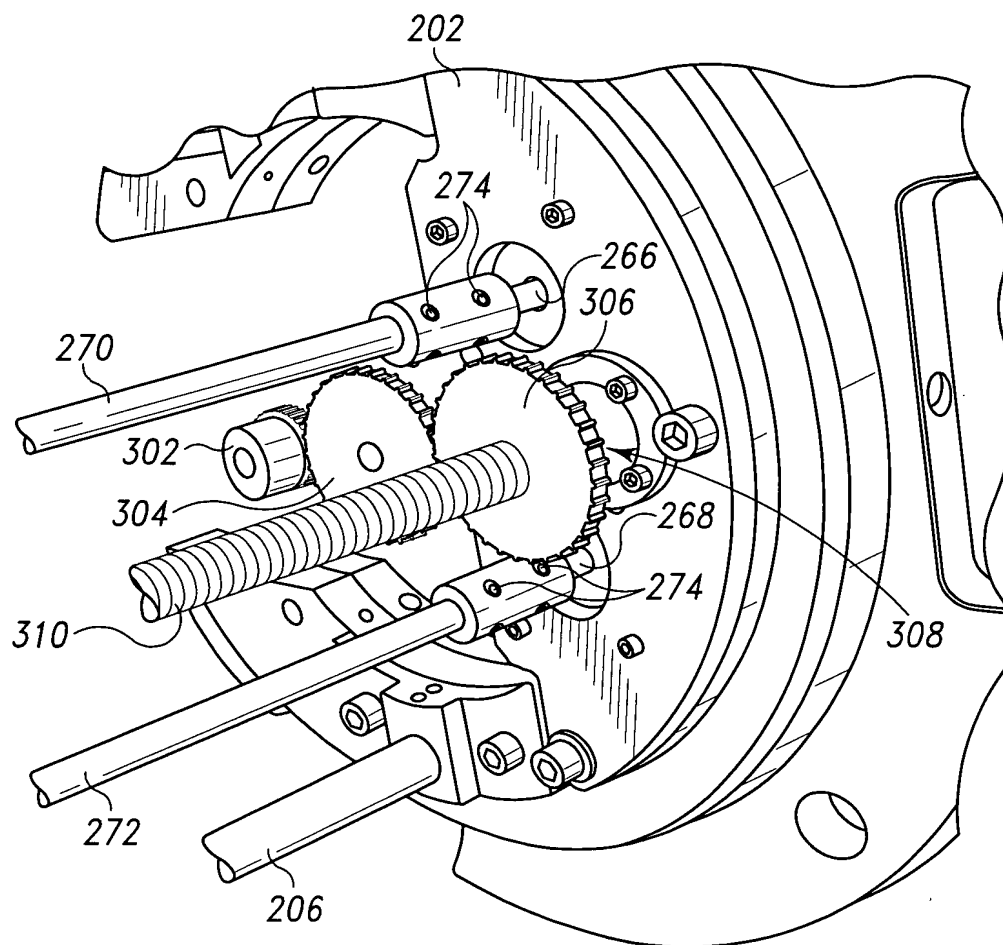


Fig. 26

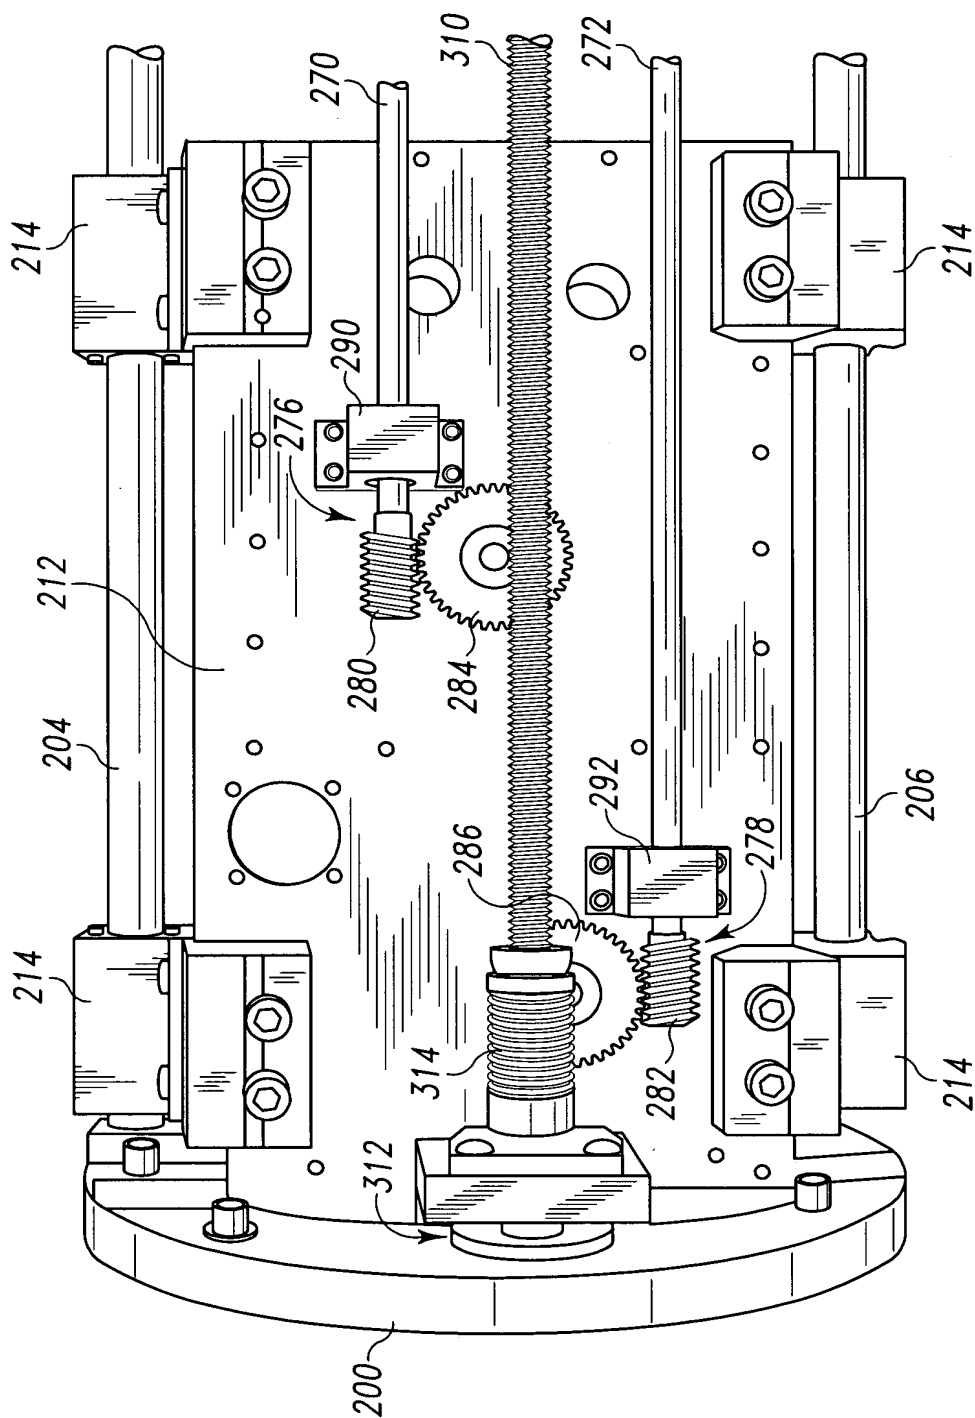


Fig. 27

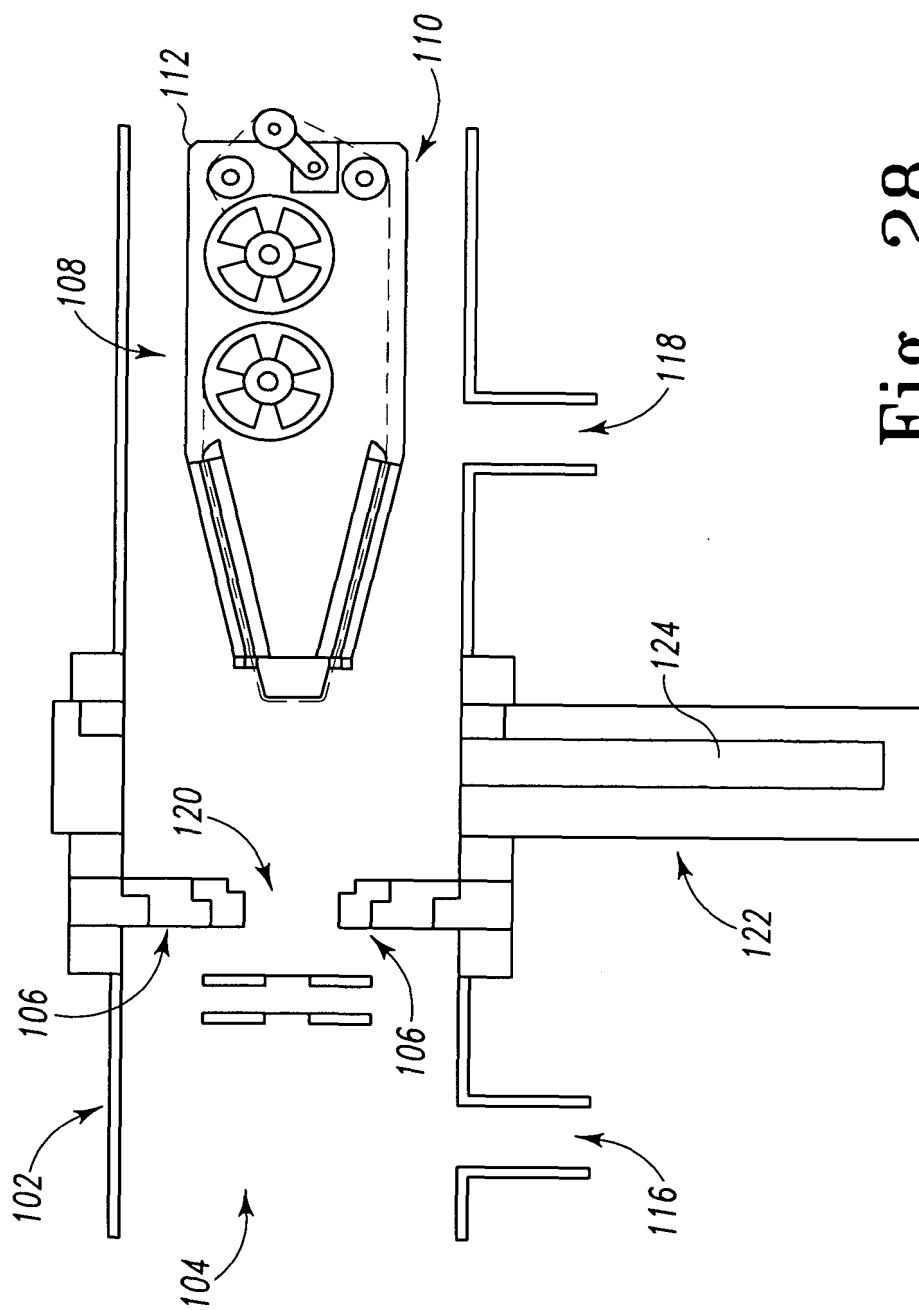


Fig. 28

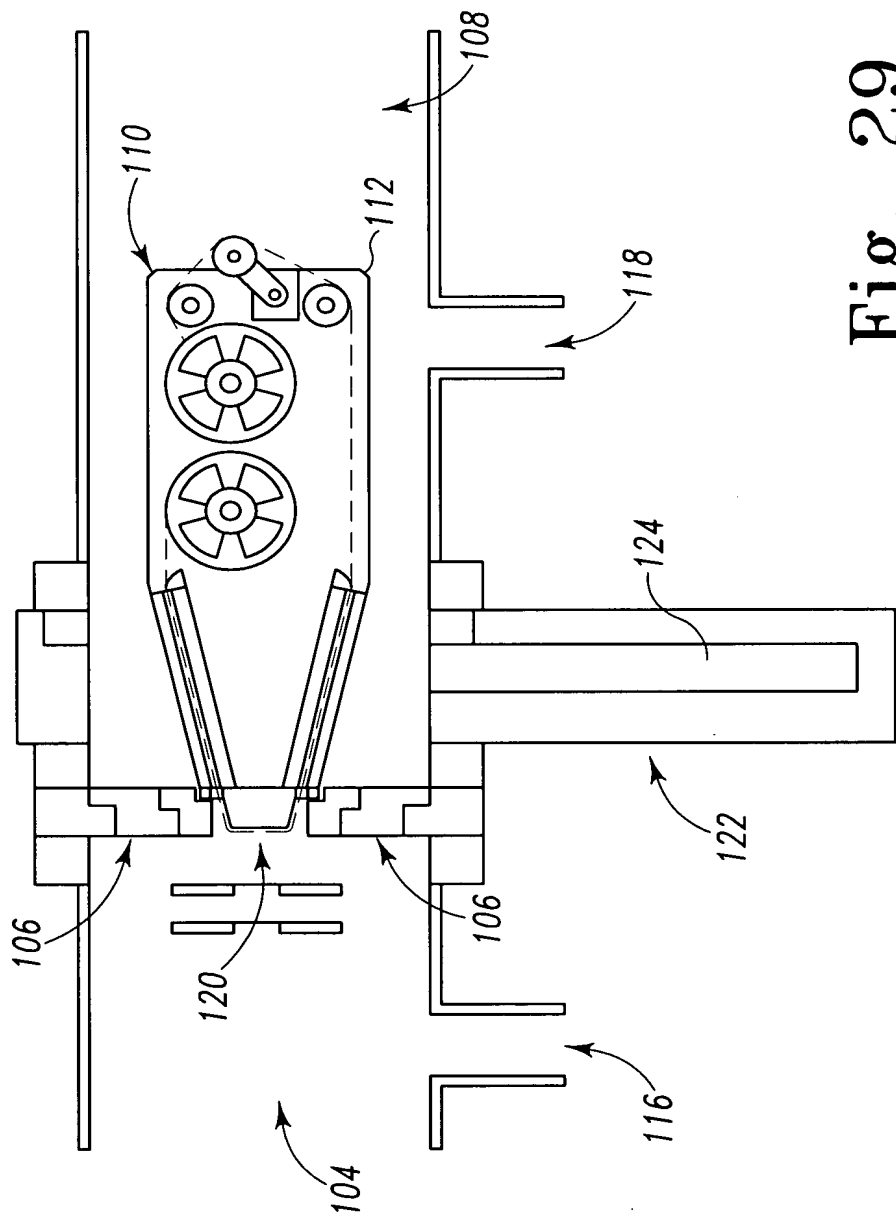


Fig. 29

